

Yocom-McColl Testing Laboratories, Inc.
 540 West Elk Place • Denver, Colorado 80216-1823 USA
 PHONE (303) 294-0582 • FAX (303) 295-6944
 EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA100)
 Micron Test Report**

Maine's Bellemont Farm Alpacas/Gay De Hart
 301 Robinson Hill Road
 Oxford ME 04270 USA

07/02/07


Test No: 297794

Animal and Sample Description

Animal Name: Don's Bellemont Skye	Animal ID: 30472877
Breed: Alpaca(Huacaya)	Sample Location: Side
Sex: Female	Sample Date: 05/03/07
Color: Light Fawn	Age: 09/11/04

Laboratory Data

Mean Fiber Diameter: 23.2 microns	Spin Fineness: 23.6 microns
Standard Deviation: 5.9 microns	Mean Curvature (deg/mm): 28.7
Coefficient of Variation: 25.5 %	SD Curvature (deg/mm): 20.3
Fibers Greater Than 30 microns: 8.4 %	
Medullated Fibers: 18.9 %	

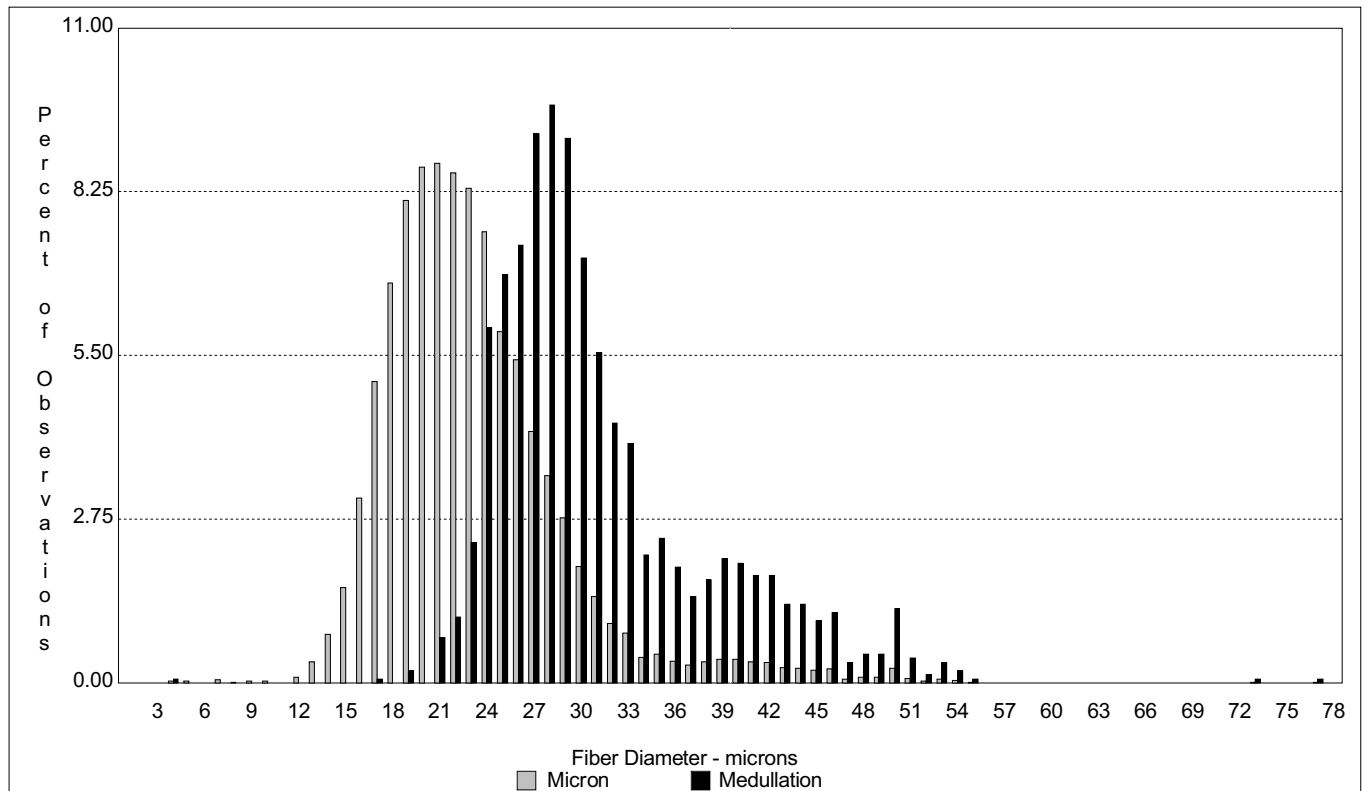

This Test Performed According to I.W.T.O Method 47